



REPORT OF CALIBRATION

DESCRIPTION: BINOCULAR TRANSMISSION

MODEL: ELITE 8X43mm

SERIAL NUMBER: 62-4208

MANUFACTURER: BUSHNELL

TECHNICIAN: FLJ

CALIBRATION DATE: 01/06/2006

RECALL DATE: 01/06/2007

CUSTOMER: CARSON OPTICAL, INC

SALES ORDER / RMN: 23876/7282

TEMP (°C): 23

REL. HUMIDITY (%): 43

PROCEDURE:

The transmittance of this Binocular was measured on a Gamma Scientific C-11 spectroradiometer configured with a Model NM-7DH double grating monochromator. A special fixture consisting of a RS-20-51 Collimated Projection Light Source, holder, and 4" diameter integrating sphere attached to DC-49C Thermoelectrically cooled Photomultiplier Detector was used to obtain the transmittance of the Binocular. The transmittance is determined by dividing the measured photocurrent values given in A to D counts of the source into the photocurrent values taken with the Binocular between the integrating sphere and the exit port of the RS-20-51 Light Source. The optical alignment of the binocular with respect to the measurement system's optical axis is directly related to measurement uncertainty.

INCOMING INSPECTION: NEW UNIT

RESULTS (Average Transmittance covering the spectral range from 400.0nm to 700.0nm in 5.0nm step increments.):

Left Transmittance (400-700 nm) = 85.60 Right Transmittance (400-700 nm) = 85.91

The spectral transmittance values are given in the attached listing and shown in the attached plot. The data are also saved to disk file in two different ASCII text formats, EXCEL and LightTouch.

All calibrations are performed using internationally recognized standards calibrated by the National Institute of Standards and Technology (NIST) for use at Gamma Scientific. The NIST test numbers for each standard used are listed below. The test equipment used to determine acceptance of Gamma Scientific products is maintained at the level of accuracy to ensure complete compliance with ANSI/NC SL Z540-1-1994. The information shown on this certificate applies only to the instrument identified above and may not be reproduced, except in full, without prior written consent from Gamma Scientific.

SPECIAL NOTES: Calibrated to ISO 14490 and ISO 8478.

A 3.00 percent variance in transmittance of the binoculars, including Left and Right optics, may be attributed to differences in optical components and the lens coatings applied.

Quality Assurance

STANDARDS USED: GS-1015 1000 WATT LAMP
NIST TEST#: 844/269328-03
DR-13 CANDELA STANDARD
NIST TEST #: 844/271329-05/2

ACCEPT	REJECT

Title: BUSHNELL ELITE 8X42MM LEFT TRANSMITTANCE FINAL 01/06/06
Date/Time: 01-05-2006 / 23:03:41
Standard/Reference Illuminant applied: 5000-16C 1000 W FEL LAMP S/N: GS-1015 / None
Units: % Transmittance, N/A
Hardware: NM-23 200-1700nm,RS-20-51,NM-7DH 290-1110nm,DC-49C 350-1010nm, (N/A)
Notes:
Number of points: 95
X-Axis-Low,High,Step: 360, 830, 5 / Y-Axis-Low,High: 9.7029e-01, 9.2768e+01

(Ir)Radiance/Photon (Ir)Radiance/Integral
Integral: 3.174e+02 / Photon Integral: 9.256e+14

Tristimulus (CIE 1931, 2° observer)
X=8.849e+01 Y=8.843e+01 Z=8.013e+01

Chromaticity (CIE 1931 xy and CIE 1976 UCS u'v')
x=0.3443 y=0.3440 u'=0.2138 v'=0.4808

Color Space (CIE 1976 L*u*v* and CIE 1976 L*a*b*)
L*=9.534e+01 u*=4.107e+00 v*=8.810e+00 a*=1.159e-01 b*=6.205e+00

(Il)Luminance
No luminance or illuminance value.

Correlated Color Temperature/MPCD
1.997e+02 Mk⁻¹ 5.006e+03 Kelvin / 10.0 MPCDs

Tristimulus (CIE 1964, 10° observer)
X=8.827e+01 Y=8.804e+01 Z=7.971e+01

Chromaticity (CIE 1964 xy)
x=0.3448 y=0.3439


LED - Illuminant E
Dominant WL 578.3 / Peak WL 660.00 / Luminous Intensity @ 10 cm (cd) 0.000e+00

Title: BUSHNELL ELITE 8X42MM LEFT TRANSMITTANCE FINAL 01/06/06
 Date/Time: 01-05-2006 / 23:03:41
 Standard/Reference Illuminant applied: 5000-16C 1000 W FEL LAMP S/N: GS-1015 / None
 Units: % Transmittance, N/A
 Hardware: NM-23 200-1700nm,RS-20-51,NM-7DH 290-1110nm,DC-49C 350-1010nm, (N/A)
 Notes:
 Number of points: 95
 X-Axis-Low,High,Step: 360, 830, 5 / Y-Axis-Low,High: 9.7029e-01, 9.2768e+01

0360.0 nm	9.7029e-01	0610.0 nm	9.1416e+01
0365.0 nm	3.6234e+00	0615.0 nm	9.1156e+01
0370.0 nm	8.9312e+00	0620.0 nm	9.1578e+01
0375.0 nm	1.6899e+01	0625.0 nm	9.2562e+01
0380.0 nm	2.5654e+01	0630.0 nm	9.2362e+01
0385.0 nm	3.5516e+01	0635.0 nm	9.2022e+01
0390.0 nm	4.4713e+01	0640.0 nm	9.1871e+01
0395.0 nm	5.3031e+01	0645.0 nm	9.2134e+01
0400.0 nm	5.9700e+01	0650.0 nm	9.2616e+01
0405.0 nm	6.5242e+01	0655.0 nm	9.2048e+01
0410.0 nm	6.9354e+01	0660.0 nm	9.2768e+01
0415.0 nm	7.2534e+01	0665.0 nm	9.2012e+01
0420.0 nm	7.5099e+01	0670.0 nm	9.1298e+01
0425.0 nm	7.6592e+01	0675.0 nm	9.0256e+01
0430.0 nm	7.7821e+01	0680.0 nm	9.0034e+01
0435.0 nm	7.8799e+01	0685.0 nm	8.9295e+01
0440.0 nm	7.9367e+01	0690.0 nm	8.8534e+01
0445.0 nm	7.9806e+01	0695.0 nm	8.6400e+01
0450.0 nm	8.0614e+01	0700.0 nm	8.5638e+01
0455.0 nm	8.1030e+01	0705.0 nm	8.2273e+01
0460.0 nm	8.1894e+01	0710.0 nm	7.8044e+01
0465.0 nm	8.1814e+01	0715.0 nm	7.5429e+01
0470.0 nm	8.2067e+01	0720.0 nm	7.1856e+01
0475.0 nm	8.2488e+01	0725.0 nm	6.7052e+01
0480.0 nm	8.2661e+01	0730.0 nm	5.9215e+01
0485.0 nm	8.2428e+01	0735.0 nm	4.6866e+01
0490.0 nm	8.2353e+01	0740.0 nm	3.5476e+01
0495.0 nm	8.4008e+01	0745.0 nm	2.8921e+01
0500.0 nm	8.4548e+01	0750.0 nm	2.7906e+01
0505.0 nm	8.5360e+01	0755.0 nm	2.8317e+01
0510.0 nm	8.5998e+01	0760.0 nm	2.7196e+01
0515.0 nm	8.6003e+01	0765.0 nm	2.3444e+01
0520.0 nm	8.6347e+01	0770.0 nm	2.0327e+01
0525.0 nm	8.6824e+01	0775.0 nm	2.0197e+01
0530.0 nm	8.7634e+01	0780.0 nm	2.1663e+01
0535.0 nm	8.8087e+01	0785.0 nm	2.1854e+01
0540.0 nm	8.7545e+01	0790.0 nm	2.1232e+01
0545.0 nm	8.8102e+01	0795.0 nm	1.9506e+01
0550.0 nm	8.7833e+01	0800.0 nm	1.8258e+01
0555.0 nm	8.7606e+01	0805.0 nm	1.8513e+01
0560.0 nm	8.8207e+01	0810.0 nm	1.9544e+01
0565.0 nm	8.9298e+01	0815.0 nm	2.1459e+01
0570.0 nm	8.9434e+01	0820.0 nm	2.4126e+01
0575.0 nm	8.9692e+01	0825.0 nm	2.7814e+01
0580.0 nm	8.9521e+01	0830.0 nm	3.0117e+01
0585.0 nm	8.9854e+01		
0590.0 nm	8.9905e+01		
0595.0 nm	9.0195e+01		
0600.0 nm	9.0651e+01		
0605.0 nm	9.1248e+01		

Gamma Scientific Test No: N/A

BUSHNELL ELITE 8X42MM LEFT TRANSMITTANCE FINAL 01/06/06

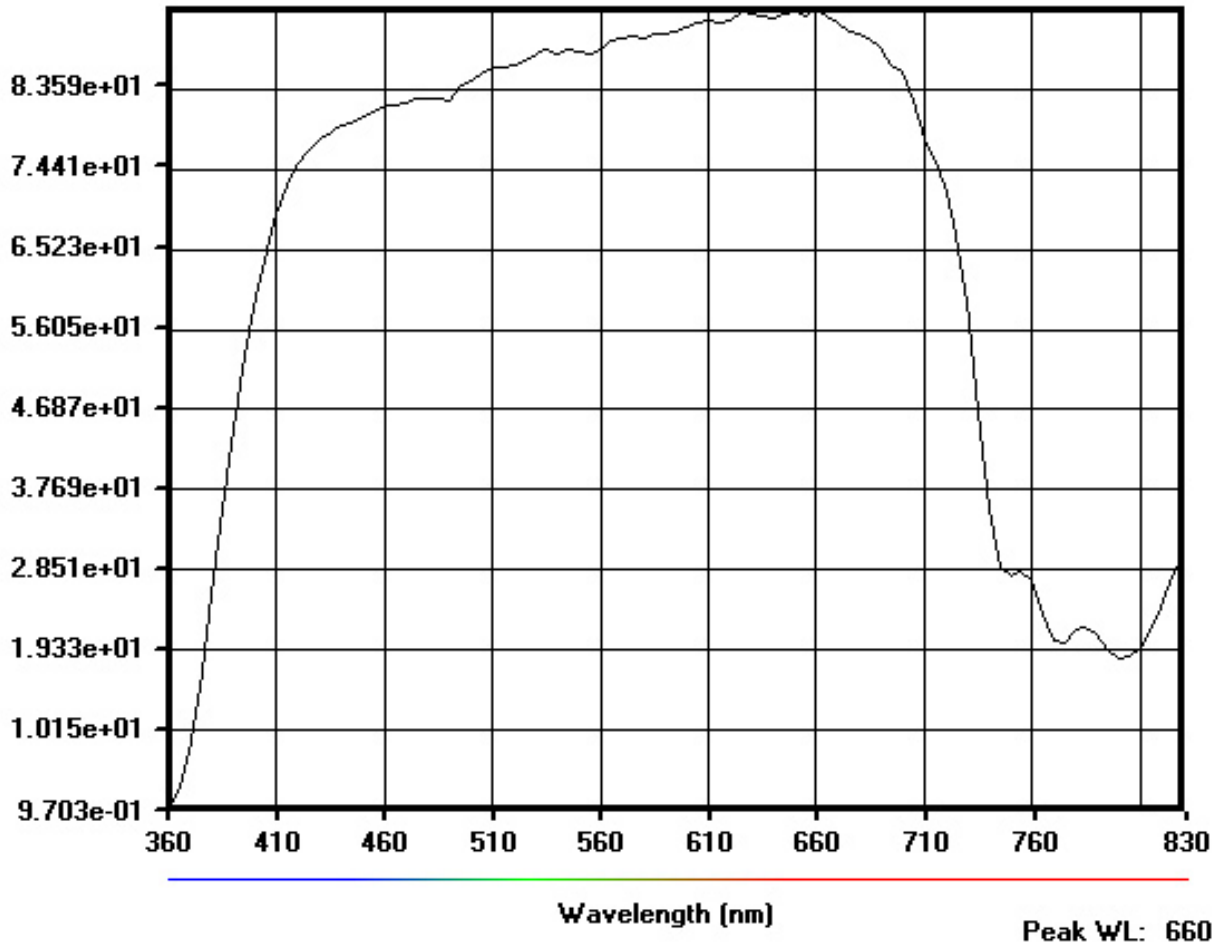

Title: BUSHNELL ELITE 8X42MM RIGHT TRANSMITTANCE FINAL 01/06/06
Date/Time: 01-05-2006 / 22:43:18
Standard/Reference Illuminant applied: 5000-16C 1000 W FEL LAMP S/N: GS-1015 / None
Units: % Transmittance, N/A
Hardware: NM-23 200-1700nm,RS-20-51,NM-7DH 290-1110nm,DC-49C 350-1010nm, (N/A)
Notes:
Number of points: 95
X-Axis-Low,High,Step: 360, 830, 5 / Y-Axis-Low,High: 1.0984e+00, 9.2339e+01

(Ir)Radiance/Photon (Ir)Radiance/Integral
Integral: 3.209e+02 / Photon Integral: 9.360e+14

Tristimulus (CIE 1931, 2° observer)
X=8.882e+01 Y=8.854e+01 Z=8.135e+01

Chromaticity (CIE 1931 xy and CIE 1976 UCS u'v')
x=0.3433 y=0.3422 u'=0.2139 v'=0.4798

Color Space (CIE 1976 L*u*v* and CIE 1976 L*a*b*)
L*=9.539e+01 u*=4.181e+00 v*=7.526e+00 a*=5.054e-01 b*=5.344e+00

(Il)Luminance
No luminance or illuminance value.

Correlated Color Temperature/MPCD
1.985e+02 Mk⁻¹ 5.039e+03 Kelvin / 11.5 MPCDs

Tristimulus (CIE 1964, 10° observer)
X=8.861e+01 Y=8.818e+01 Z=8.100e+01

Chromaticity (CIE 1964 xy)
x=0.3437 y=0.3421

LED - Illuminant E
Dominant WL 579.4 / Peak WL 640.00 / Luminous Intensity @ 10 cm (cd) 0.000e+00

Title: BUSHNELL ELITE 8X42MM RIGHT TRANSMITTANCE FINAL 01/06/06

Date/Time: 01-05-2006 / 22:43:18

Standard/Reference Illuminant applied: 5000-16C 1000 W FEL LAMP S/N: GS-1015 / None

Units: % Transmittance, N/A

Hardware: NM-23 200-1700nm,RS-20-51,NM-7DH 290-1110nm,DC-49C 350-1010nm, (N/A)

Notes:

Number of points: 95

X-Axis-Low,High,Step: 360, 830, 5 / Y-Axis-Low,High: 1.0984e+00, 9.2339e+01

0360.0 nm	1.0984e+00	0610.0 nm	9.1998e+01
0365.0 nm	3.9267e+00	0615.0 nm	9.1601e+01
0370.0 nm	9.5570e+00	0620.0 nm	9.1730e+01
0375.0 nm	1.7831e+01	0625.0 nm	9.1828e+01
0380.0 nm	2.6759e+01	0630.0 nm	9.2145e+01
0385.0 nm	3.6504e+01	0635.0 nm	9.1966e+01
0390.0 nm	4.6593e+01	0640.0 nm	9.2339e+01
0395.0 nm	5.4553e+01	0645.0 nm	9.2012e+01
0400.0 nm	6.1359e+01	0650.0 nm	9.1852e+01
0405.0 nm	6.6975e+01	0655.0 nm	9.1518e+01
0410.0 nm	7.1061e+01	0660.0 nm	9.1864e+01
0415.0 nm	7.4402e+01	0665.0 nm	9.0704e+01
0420.0 nm	7.6901e+01	0670.0 nm	9.0458e+01
0425.0 nm	7.8506e+01	0675.0 nm	8.9617e+01
0430.0 nm	7.9865e+01	0680.0 nm	8.9020e+01
0435.0 nm	8.0461e+01	0685.0 nm	8.8582e+01
0440.0 nm	8.1011e+01	0690.0 nm	8.7500e+01
0445.0 nm	8.1350e+01	0695.0 nm	8.6300e+01
0450.0 nm	8.1831e+01	0700.0 nm	8.4681e+01
0455.0 nm	8.2434e+01	0705.0 nm	8.3182e+01
0460.0 nm	8.3070e+01	0710.0 nm	7.9372e+01
0465.0 nm	8.3006e+01	0715.0 nm	7.7117e+01
0470.0 nm	8.2723e+01	0720.0 nm	7.4723e+01
0475.0 nm	8.2811e+01	0725.0 nm	7.2281e+01
0480.0 nm	8.3101e+01	0730.0 nm	6.7509e+01
0485.0 nm	8.3198e+01	0735.0 nm	5.6543e+01
0490.0 nm	8.2833e+01	0740.0 nm	4.2718e+01
0495.0 nm	8.3278e+01	0745.0 nm	3.3120e+01
0500.0 nm	8.4922e+01	0750.0 nm	3.0913e+01
0505.0 nm	8.5655e+01	0755.0 nm	3.2656e+01
0510.0 nm	8.5771e+01	0760.0 nm	3.3003e+01
0515.0 nm	8.5894e+01	0765.0 nm	2.7835e+01
0520.0 nm	8.6453e+01	0770.0 nm	2.1569e+01
0525.0 nm	8.6824e+01	0775.0 nm	1.8977e+01
0530.0 nm	8.7045e+01	0780.0 nm	1.9777e+01
0535.0 nm	8.7629e+01	0785.0 nm	2.0611e+01
0540.0 nm	8.8026e+01	0790.0 nm	2.0448e+01
0545.0 nm	8.7580e+01	0795.0 nm	1.9320e+01
0550.0 nm	8.7728e+01	0800.0 nm	1.7930e+01
0555.0 nm	8.8169e+01	0805.0 nm	1.7635e+01
0560.0 nm	8.8648e+01	0810.0 nm	1.9610e+01
0565.0 nm	8.9469e+01	0815.0 nm	2.1261e+01
0570.0 nm	8.9434e+01	0820.0 nm	2.1631e+01
0575.0 nm	8.9861e+01	0825.0 nm	2.3799e+01
0580.0 nm	9.0157e+01	0830.0 nm	2.7573e+01
0585.0 nm	9.0197e+01		
0590.0 nm	9.0128e+01		
0595.0 nm	9.0495e+01		
0600.0 nm	9.1036e+01		
0605.0 nm	9.1153e+01		

Gamma Scientific Test No: N/A

BUSHNELL ELITE 8X42MM RIGHT TRANSMITTANCE FINAL 01/06/06

